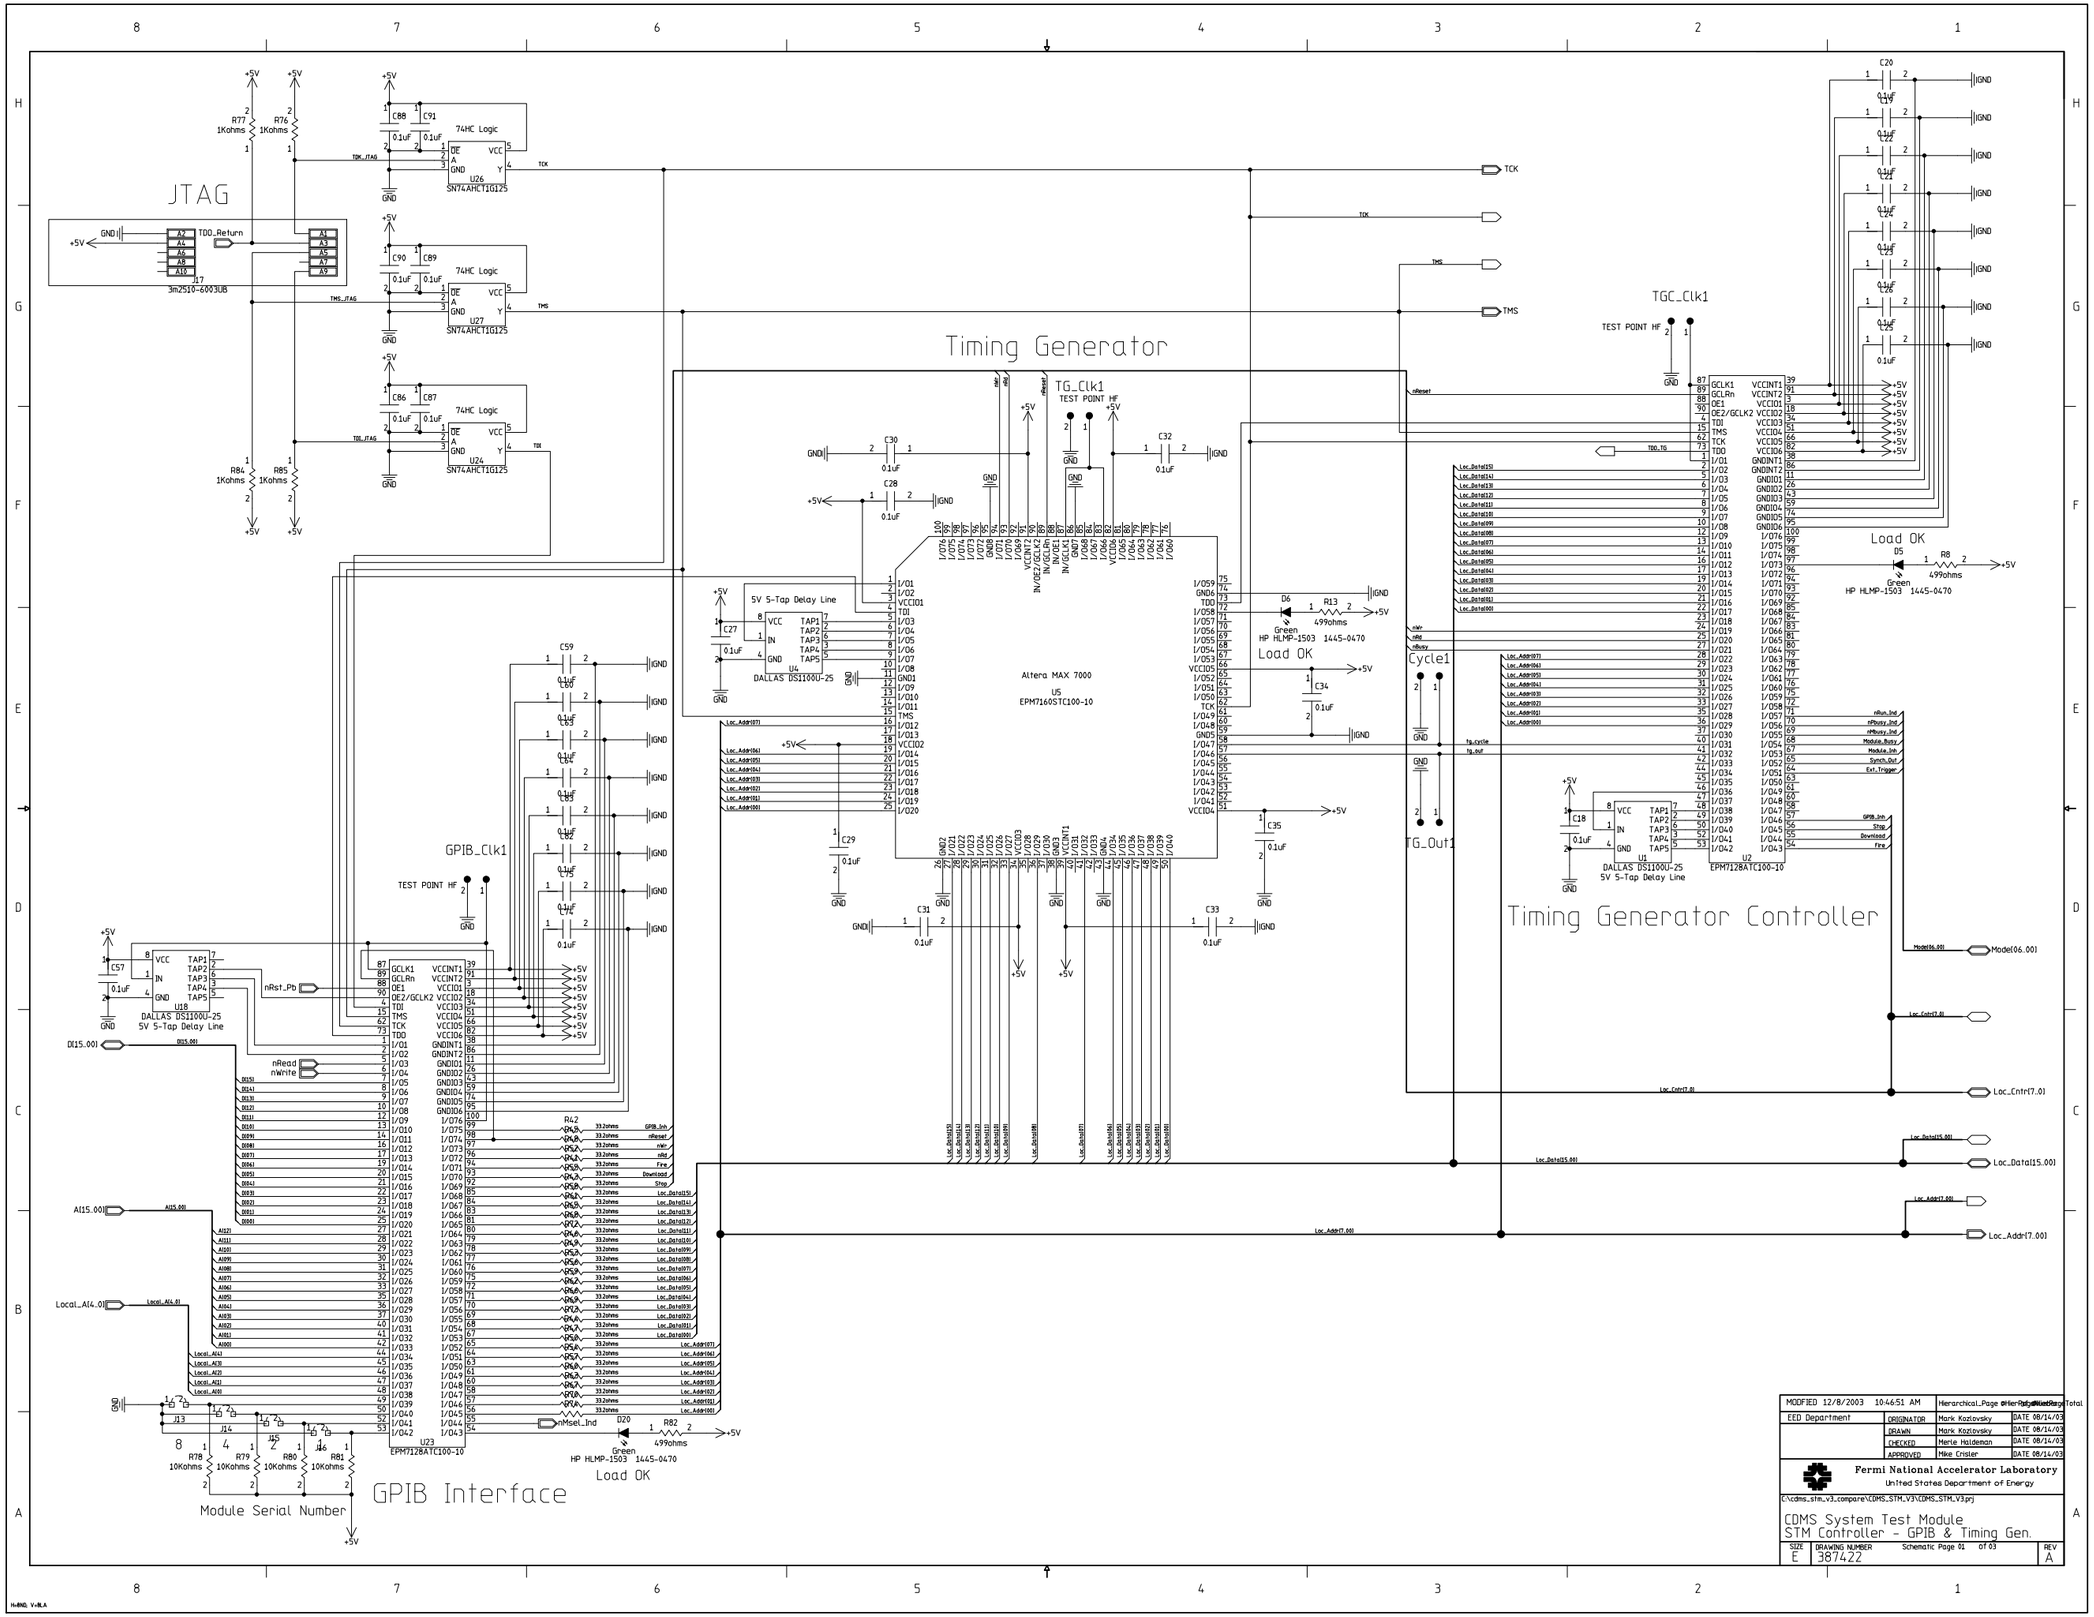
JTAG
3m2510-6003UB
74HC Logic
SN74AHCT1G125
Timing Generator
Altera MAX 7000
U5
EPM7160STC100-10
5V 5-Tap Delay Line
DALLAS DS1100U-25
TG_Clk1
TEST POINT HF
Load OK
Green
HP HLMP-1503 1445-0470
499ohms
Cycle1
TG_Out1
TGC_Clk1
EPM7128ATC100-10
Timing Generator Controller
GPIB_Clk1
GPIB Interface
Module Serial Number
10Kohms
Mode(06.00)
Loc_Cntr(7.0)
Loc_Data(15.00)
Loc_Addr(7.00)
MODIFIED 12/8/2003 10:46:51 AM
EED Department
ORIGINATOR Mark Kozlovsky DATE 08/14/03
DRAWN Mark Kozlovsky DATE 08/14/03
CHECKED Merle Haldeman DATE 08/14/03
APPROVED Mike Crisler DATE 08/14/03
Fermi National Accelerator Laboratory
United States Department of Energy
C:\cdms_stm_v3_compare\CDMS_STM_V3\CDMS_STM_V3.prj
CDMS System Test Module
STM Controller - GPIB & Timing Gen.
SIZE E
DRAWING NUMBER 387422
Schematic Page 01 of 03
REV A